

Please read instructions for use carefully before starting the assay

CENP-A ELISA

ELISA for the semi-quantitative determination of anti-CENP-A antibodies in human serum and plasma

REF 25024 Σ 96 Determinations

BACKGROUND

Anti-centromere antibodies (ACA) are found in 20-50% of patients with systemic sclerosis (SSc) and especially in patients with the CREST Syndrom (calcinosis, Raynaud phenomenon, esophageal dysmotility, sclerodactyly, and telangiectasia). The precise prevalence of ACA depends on the detection system and on the selection of the patient cohort. Furthermore, ACA are found in patients with systemic lupus erythematosus (SLE), primary biliary cirrhosis (PBC) and rheumatoid arthritis (RA), however with lower prevalence. The CENP-A ELISA is the first assay for the detection of ACA which uses a highly specific peptide sequence (patented) from the N-terminal part of CENP-A and therefore reaches a significantly higher specificity compared to common ACA assays.

INTENDED USE

The CENP-A ELISA is intended for the semi-quantitative determination of antibodies specific for the CENP-A protein. The results of the CENP-A ELISA aid to the diagnosis of systemic sclerosis and related autoimmune disorders and should be used as prognostic marker for the disease progression.

PRINCIPLE

The CENP microtiter ELISA plates are coated with synthetic CENP-A antigen. Initially, diluted patient samples (1:101), Controls and the Calibrator (undiluted) are applied to the microtiter wells. This leads to the binding of anti-CENP antibodies to the immobilized CENP antigen. After washing an anti-IgG horseradish peroxidase (HRP) conjugate is added which binds to the anti-CENP antibodies. Unbound material is removed by another washing cycle. Finally the binding of anti-CENP antibodies is visualized by incubation with TMB Substrate resulting in the development of a blue colour turning into yellow after stopping the reaction with Stop Solution.

The optical density of the yellow colour is directly proportional to the amount of bound anti-CENP antibodies and can be measured spectrophotometrically at 450 nm.

A Calibrator with a known concentration of anti-CENP antibodies is tested simultaneously with the samples. Semi-quantitative results can be determined by calculating the ratios from the OD value of the Calibrator and the samples.

KIT COMPONENTS

| | | |
|---|---|------------------------|
| Microtiter strips, antigen coated | MICROWELL | 12 strips x 8 wells |
| Anti-IgG HRP-Conjugate | CONJ HRP G | 1 x 15 mL |
| Concentrated Washing Buffer | WASHBUF B 25x | 1 x 50 mL |
| TMB Substrate | SUB TMB | 1 x 15 mL |
| Stop Solution (0.5 M H ₂ SO ₄) | STOP H₂SO₄ | 1 x 12 mL |
| Dilution Buffer | DILBUF B | 1 x 60 mL |
| Calibrator | CAL | 1 x 2 mL |
| Negative Control | CONTROL - | 1 x 2 mL |
| Positive Control | CONTROL + | 1 x 2 mL |

MATERIAL NEEDED, BUT NOT PROVIDED WITH THE KIT

2-10 µL, 10-100 µL and 200-1000 µL pipettes, Multipipette, pipet tips, vials for diluting the specimen, graduated glass cylinder, lab watch, microplate-reader, covering foil, microplate-washer (optional).

SPECIMEN COLLECTION & PREPARATION

Either Serum or Plasma can be used in this test. No additives or preservatives are necessary to maintain the integrity of the specimen.

Specimens should be stored at 2-8°C and assayed within 48 hours after collection. If the assay cannot be performed within 48 hours or if the specimen has to be shipped, cap the specimen and keep it frozen. Repeated freezing and thawing should be avoided. Frozen specimens should be thawed at room temperature (RT, 20-25°C) and mixed thoroughly by gentle inversion before assaying. The use of haemolysed or lipemic specimens is not recommended.

PREPARATION OF REAGENTS

Allow all reagents to come to RT before use. Unused microtiterstrips have to be resealed properly in the provided foil bag containing a desiccant.

Dilution Buffer: ready to use
HRP Conjugate: ready to use
Substrate Solution: ready to use
Stop Solution: ready to use
Calibrator and Controls: ready to use
Concentrated Washing Buffer:


The Concentrated Washing Buffer has to be diluted 1:25 in aqua bidest. (Example: One strip requires 40 mL of Washing Buffer, therefore 1.6 mL Concentrated Washing Buffer have to be diluted to a final volume of 40 mL with aqua bidest.). The resulting Washing Buffer is stable for one week at RT.

ASSAY PROCEDURE

1. Create a pipetting scheme. It is a must to test the Calibrator in duplicate and this is highly recommended for Controls.
2. Dilute patient samples **1:101** in Dilution Buffer (10 µL serum + 1 mL Dilution Buffer for double determination / 5 µL serum + 0.5 mL Dilution Buffer for single determination).
3. Place the required coated wells into a frame. Properly reseal the aluminium bag with the remaining strips and desiccant.
4. Pipette 100 µL of Calibrators, Controls and diluted patient samples into the antigen coated wells according to the pipetting scheme.
5. Cover the plate and incubate for 30 min at RT.
6. Wash the plate manually or with an appropriate ELISA plate washer at least 3 times with minimally 300 µL per well. Remove residual liquid by dunking the microplate on a tissue.

7. Add 100 µL of anti-IgG HRP conjugate to all wells. Cover the plate and incubate for 30 min at room temperature.
8. Repeat washing procedure as described in step 6.
9. Add 100 µL of TMB Substrate to each well, cover the plate and incubate for 15 min at RT (TMB substrate is light sensitive).
10. Pipette 50 µL of Stop Solution in the same order as the substrate to each well. It is recommended to mix the solution in the wells by carefully knocking on the frame. Read OD at 450 nm (reference wave length 620 nm*) using an appropriate microplate reader and calculate the results of patient samples and controls as described on page 3.

TESTING SCHEME AI-LINE ELISA

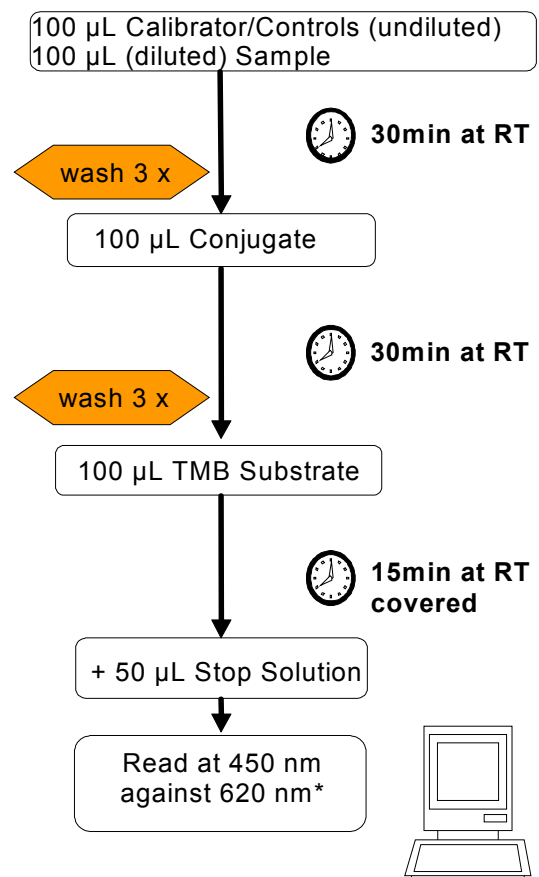

* The measurement against the reference wave length from 620 nm is optional.



DR. FOOKE

Laboratorien GmbH Tel. : 0049-2131-2984-0
 Habichtweg 16 Fax : 0049-2131-2984-184
 4 1 4 6 8 Neuss
 E-mail: information@fooke-labs.de
 Internet: www.fooke-labs.de

CALCULATION OF RESULTS

Calculate the ratios between the OD value [Δ 450 nm – 620 nm] of each patient sample and the mean OD value [450 nm] of the Calibrator. Do the same for the controls. Multiply all obtained ratios by the conversion factor (F). This conversion factor is lot specific and is stated on the Quality Control Certificate. Resulting values are expressed as relative units (RU).

Calculation:

$$RU \text{ sample} = \frac{OD \text{ Sample}}{OD \text{ Calibrator}} \times F$$

Example:

OD Calibrator = 1.9
OD Sample = 0.6
Conversion factor F = 10

$$RU \text{ sample} = \frac{OD \text{ Sample}}{OD \text{ Calibrator}} \times 10$$

$$RU \text{ sample} = \frac{0.6}{1.9} \times 10$$

$$RU \text{ sample} = 3.2 \text{ RU}$$

RESULT INTERPRETATION

For interpretation of the results use the following cut-off values.

< 1 RU Negative
1-1.5 RU Borderline
> 1.5 RU Positive

The cut-off values were determined using disease controls and normal sera.

VALIDATION CRITERIA

The OD value of the Calibrator and the RU values of the Controls have to meet the ranges stated on the QC-Certificate. Otherwise, the test conditions should be verified and the test should probably be repeated.

REFERENCE RANGES

The average value of samples from apparently healthy controls was found at 0.4 RU (Standard Deviation 0.2 RU). Each laboratory should establish its own reference ranges.

MEASURING RANGE

0.1 up to 7.5 relative units (RU).

PRECISION

Variability and reproducibility was evaluated with three different positive sera. The Intra-assay variability for a quadruplicate measurement was below 6%. The Inter-assay variability, determined with duplicates taken from seven different runs, was below 13%.

SPECIFICITY

The diagnostic specificity for SSc tested against various autoimmune disorders was found at 97.1%.

SENSITIVITY

The diagnostic sensitivity for SSc tested against various autoimmune disorders was found at 45.7%.

LITERATURE

1. Tan EM: **Antinuclear antibodies: diagnostic markers for autoimmune diseases and probes for cell biology.** *Adv Immunol* 1989, **44**:93-151.
2. James K, Carpenter AB, Cook L, Marchand R, and Nakamura RM for the Association of Medical Laboratory Immunologists Standards Committee: **Development of the Antinuclear and Anti-cytoplasmic Antibody Consensus Panel by the Association of Medical Laboratory Immunologists.** *Clin Diagn Lab Immunol* 2000, **7**:436–443.
3. Fritzler MJ, Kinsella TD: **The CREST syndrome: a distinct serologic entity with anticentromere antibodies.** *Am J Med* 1980, **69**:520-526.
4. Earnshaw WC, Machlin PS, Bordwell BJ, Rothfield NF, Cleveland DW: **Analysis of anticentromere autoantibodies using cloned autoantigen CENP-B.** *Proc Natl Acad Sci U S A* 1987, **84**:4979-4983.
5. Mahler M, Mierau R, Blüthner M. **Fine-specificity of the anti-CENP-A B-cell autoimmune response.** *J Mol Med* 2000, **78**:460-7.
6. Mahler M, Mierau R, Genth E, Blüthner M. **Development of a CENP-A/CENP-B-specific immune response in a patient with systemic sclerosis.** *Arthritis Rheum* 2002, **46**:1866-72.

PRECAUTIONS FOR USERS

- In compliance with article 1 paragraph 2b European directive 98/79/EC the use of *in-vitro* diagnostic medical devices is intended to secure suitability, performance and safety of the product by the manufacturer. Therefore the test procedure, information, precautions and warnings stated in the instructions for use have to be followed strictly. The kit has only to be used as described on page 1 (intended use).
- The test must be performed according to this instruction, which contains all necessary information, precautions and warnings. The use of the test kit with analyzers and similar equipment has to be validated. Any change in design, composition of the test procedure as well as for any use in combination with other products not approved by the manufacturer is not authorized; the user himself is responsible for such changes resulting in false results and other incidents. The manufacturer is not liable for any results obtained by visual analysis of patient samples.
- The kit is intended for use by trained and qualified professionals carrying out research or diagnostic activities only. Pregnant women should not perform the test.
- Laboratory equipment has to be maintained according to the manufacturer's instructions and must be tested for its correct function before use.
- For *in-vitro* diagnostic use only. Use only once. Do not use components exceeding the expiry date. Do not combine reagents of other suppliers or kit components of different lots (unless specified on page 1) with this kit.
- Do not use kit components when the package of the component is damaged. Please check all solutions prior to use for microbiological contamination. Cap vials tightly immediately after use to avoid evaporation and microbiological contamination. Do not interchange screw caps of the reagent vials.
- The kit was evaluated for use at the temperatures specified in the Testing scheme (see page 2). Higher or lower temperatures may result in values not meeting the quality control ranges.
- The washing procedure is absolutely important. Improper washing will cause erroneous results. It is recommended to use a multichannel pipette and an automated washer.
- To avoid cross-contamination and false-positive results it is recommended to perform all pipetting steps properly. Use only clean pipette tips, dispensers and lab ware.
- Test components based on human serum were tested using a CE marked method for the presence of antibodies against HIV 1 / HIV 2, Anti-HBc, and Anti-HCV as well as for hepatitis antigen HBsAg and were found to be negative. Nevertheless, material based on human serum should be handled as potentially infectious (BIOHAZARD).
- Some kit components may contain bovine serum albumin, of which according to the manufacturer no infectious potential is known. Due to the eventual occurrence of undetectable infectious agents we recommend to handle any product of animal origin as potentially infectious.
- The following safety rules should be followed with all reagents:
 - Do not get in eyes, on skin, or on clothing (P262). Do not breathe spray (P260). Pipetting should never be done by mouth, but with suitable pipetting devices.
 - IF SWALLOWED: rinse mouth. Do NOT induce vomiting (P301/330/331)
 - IF ON SKIN (or hair): Remove/Take off immediately all contaminated clothing. Rinse skin with water/shower (P303/361/353).
 - IF INHALED: Remove victim to fresh air and keep at rest in a position comfortable for breathing (P303/340).
 - IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing. (P305/351/338)
 - Don't eat, drink or smoke while performing the test. Keep away from food, feed and beverage.
 - Wear protective gloves/protective clothing/eye protection (P280). Wash hands thoroughly after handling (P264) and care for your skin.
 - Material safety data sheet is available on request.
- Stop Solution causes severe skin burns and eye damage (H314).
- TMB in high concentrations may be potentially mutagenic. Due to the low concentration of TMB in this substrate solution a mutagenic effect can be ruled out, if it is properly used.
- The preservatives (Bronidox, Thimerosal, Azid) are toxic to aquatic life, but their concentration is not hazardous to environment anymore. On disposal, flush large volumes of reagents with plenty of water. Thimerosal (WashBuf B) may cause damage to organs through prolonged or repeated exposure (H373)
- Waste containing serum must be collected in separate containers containing an appropriate disinfectant in sufficient concentration. This material has to be treated according to national biohazard and safety guidelines or regulations.
- We refer to the national regulations of medical devices regarding *in-vitro* diagnostic test kits.



DR. FOOKE

Laboratorien GmbH Tel. : 0049-2131-2984-0
 Habichtweg 16 Fax : 0049-2131-2984-184
 4 1 4 6 8 Neuss
 E-mail: information@fooke-labs.de
 Internet: www.fooke-labs.de

| | | | | | | | | | | | | |
|-------------|---------------------|------------------------------------|-------------------|------------|------------------|------------------------------|------------------------------|------------------------------------|---------------|--------------------------|-----------------|------------|
| | | | | | | | | | | | | |
| Lot- Number | European conformity | For <i>in-vitro</i> diagnostic use | Temperature Limit | Use before | Catalogue Number | Consult instructions for use | Refer accompanying documents | Do not use when package is damaged | Do not Re-use | Sufficient for <n> tests | Manufactured by | Bio-hazard |